



**LABORATORY FOR TESTING OF MACHINERY,
EQUIPMENT AND DEVICES**
CENTER FOR TESTING AND EUROPEAN CERTIFICATION LTD

2, Industrialna Str., Stara Zagora, Bulgaria,
Tel.: +359 42 620 368 Fax: +359 42 602 377 ctec@ctec-sz.com

TEST REPORT

№ Zemc-i-13-663 / 18.06.2013

OBJECT TO BE TESTED: Group luminaries – Industrial lighting “Bell reflector” fixtures cat. № 98A 19036SCH
Representative sample from Bell reflector fixture group with cat. №: 98A 22021SCH; 98A 22022SCH; 98A 22023SCH;
98A 22024SCH; 98A 22025SCH; 98A 22026SCH; 98A 22027SCH; 98A 22028SCH; 98A 19029SCH; 98A 19030SCH;
98A 19031SCH; 98A 19032SCH; 98A 19033SCH; 98A 19034SCH; 98A 19035SCH; 98A 19036SCH; 98A 19061SCH
98A 19062SCH; 98A 19063SCH; 98A 19064SCH; 98A 19065SCH; 98A 19066SCH; 98A 19067SCH; 98A 19068SCH;
98A 16069SCH; 98A 16071SCH; 98A 16072SCH; 98A 16073SCH; 98A 16075SCH
*(name of object to be tested, type, model, quantity,
type – portable, fixed, for walling in and other)*

APPLICANT FOR TEST: “ELMARK INDUSTRIES” SC. 2 Dobrudja Blvd. Dobrich, Bulgaria ,
Tel.: 058 500 055, e-mail: denkov@elmark.bg
Application № 663 / 08.05.2013
(name of the firm – applicant, address, telephone, number and date of the test application)

STANDART:

- EN 55015:2006+A1:2007+A2:2009 Limits and methods of measurement of radio disturbance characteristics of electrical lighting and similar equipment.
- EN 61000-3-2:2006+A1:2009+A2:2009 Electromagnetic compatibility (EMC).
Part 3-2: Limits – Limits for harmonic current emissions (equipment input current ≤ 16 A per phase).
- EN 61000-3-3:2008 Electromagnetic compatibility (EMC).
Part 3-3: Limits - Limitation of voltage changes, voltage fluctuations and flicker in public low-voltage supply systems, for equipment with rated current ≤ 16 A per phase and not subject to conditional connection.
- EN 61547:2009 Equipment for general lighting purposes - EMC immunity requirements
- EN 61000-4-2:2009 Electromagnetic compatibility (EMC).
Part 4-2: Testing and measurement techniques - Electrostatic discharge immunity test
- EN 61000-4-4:2004+A1:2010 Electromagnetic compatibility (EMC).
Part 4-4: Testing and measurement techniques - Electrical fast transient/burst immunity test
- EN 61000-4-5:2006 Electromagnetic compatibility (EMC).
Part 4-5: Testing and measurement techniques - Surge immunity test
- EN 61000-4-8:2010 Electromagnetic compatibility (EMC).
Part 4-8: Testing and measurement techniques - Power frequency magnetic field immunity test
- EN 61000-4-11:2004 Electromagnetic compatibility (EMC).
Part 4-11: Testing and measurement techniques – Voltage dips, short interruptions and voltage variations immunity tests
(number and name of the standards)

DATE OF ACCEPTANCE IN THE TEST LABORATORY: 08.05.2013

YEAR OF PRODUCTION : 2013
(identification number)

MANUFACTURER: “ELMARK INDUSTRIES” SC. 2 Dobrudja Blvd. Dobrich, Bulgaria ,
Tel.: 058 500 055, e-mail: denkov@elmark.bg
(firm, trade mark, address)

DECLARED TECHNICAL DATA: Rated voltage – 230 V AC
Rated frequency – 50 Hz
Rated power – 400 W
Class I

DATE OF TEST PERFORMANCE: 28.05.2013

LABORATORY CHIEF:
/ T. Hristov /





I. Emission of Radio disturbance characteristics of electrical lighting and similar equipment

1. Radiated electromagnetic disturbances – 9kHz ÷ 30MHz

EN 55015, cl. 4.4 – Radiated electromagnetic disturbances, limits – Table 3

EN 55015, cl. 5.2.4 – Other luminaires

EN 55015, cl. 6 – Operating conditions for lighting equipment

EN 55015, cl. 6.4 – Ambient temperature: 25 °C ; Relative Humidity: 42 %.

EN 55015, cl.9.1 – Measuring arrangement and procedure


EN 55015, cl.9.2 – Indoor and outdoor luminaires

The test is performed with MHL and supply voltage: 230 V

RESULTS OF MEASUREMENT :

Frequency	Radiated electromagnetic disturbances - measured along the axis - X		
	Quasi peak - QP		
	Measuring	Margin	Limit
MHz	dB(µA)	dB(µA)	dB(µA)
0,011	33,90	54,10	88,00
0,215	22,09	31,58	53,67
0,235	19,94	32,66	52,60
0,315	12,48	36,60	49,08
0,410	17,87	28,04	45,91
0,480	16,42	27,60	44,02
0,505	13,71	29,70	43,41
1,290	8,26	23,88	32,14
1,985	2,21	24,75	26,96
2,000	1,13	25,74	26,87
2,860	4,11	18,46	22,57
3,000	-5,38	27,38	22,00
3,970	-22,62	44,62	22,00
4,965	-20,36	42,36	22,00
5,820	-12,34	34,34	22,00
20,035	-22,25	44,25	22,00

Drawing of Radiated electromagnetic disturbances - measured along the axis - X

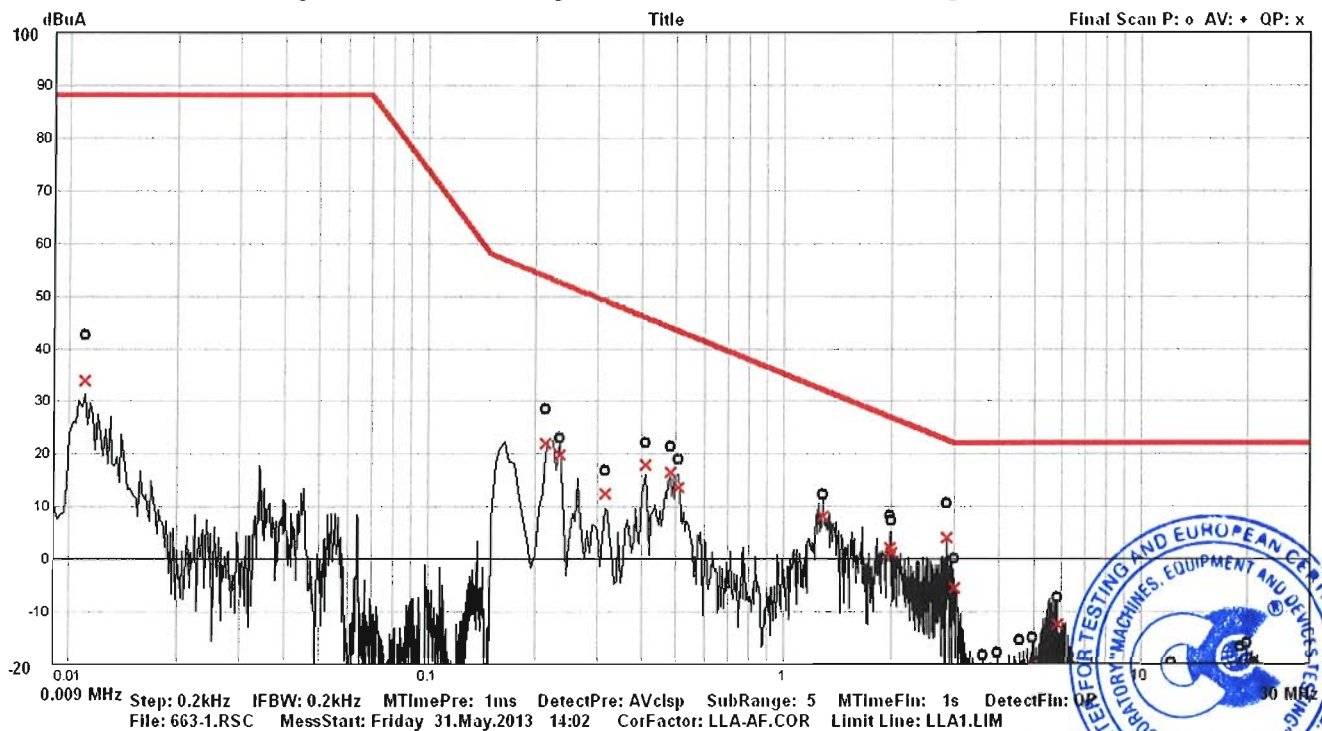

The results showed in present test report concern tested sample only

The test report could be reproduced as a whole only and after written permission of the laboratory






Radiated electromagnetic disturbances - measured along the axis - Y

Frequency

Quasi peak - QP

	Measuring	Margin	Measuring
MHz	dB(μA)	dB(μA)	dB(μA)
0,010	30,33	57,67	88,00
0,215	18,72	34,95	53,67
0,235	17,06	35,54	52,60
0,335	-1,42	49,76	48,34
0,425	13,31	32,17	45,48
0,485	9,96	33,93	43,89
0,500	12,00	31,53	43,53
1,295	-26,61	58,70	32,09
1,980	-21,54	48,53	26,99
2,040	-22,13	48,76	26,63
2,825	-12,09	34,81	22,72
3,015	-29,22	51,22	22,00
3,695	-33,58	55,58	22,00
4,155	-32,59	54,59	22,00
4,270	-33,53	55,53	22,00
20,900	-35,31	57,31	22,00

Drawing of Radiated electromagnetic disturbances - measured along the axis - Y

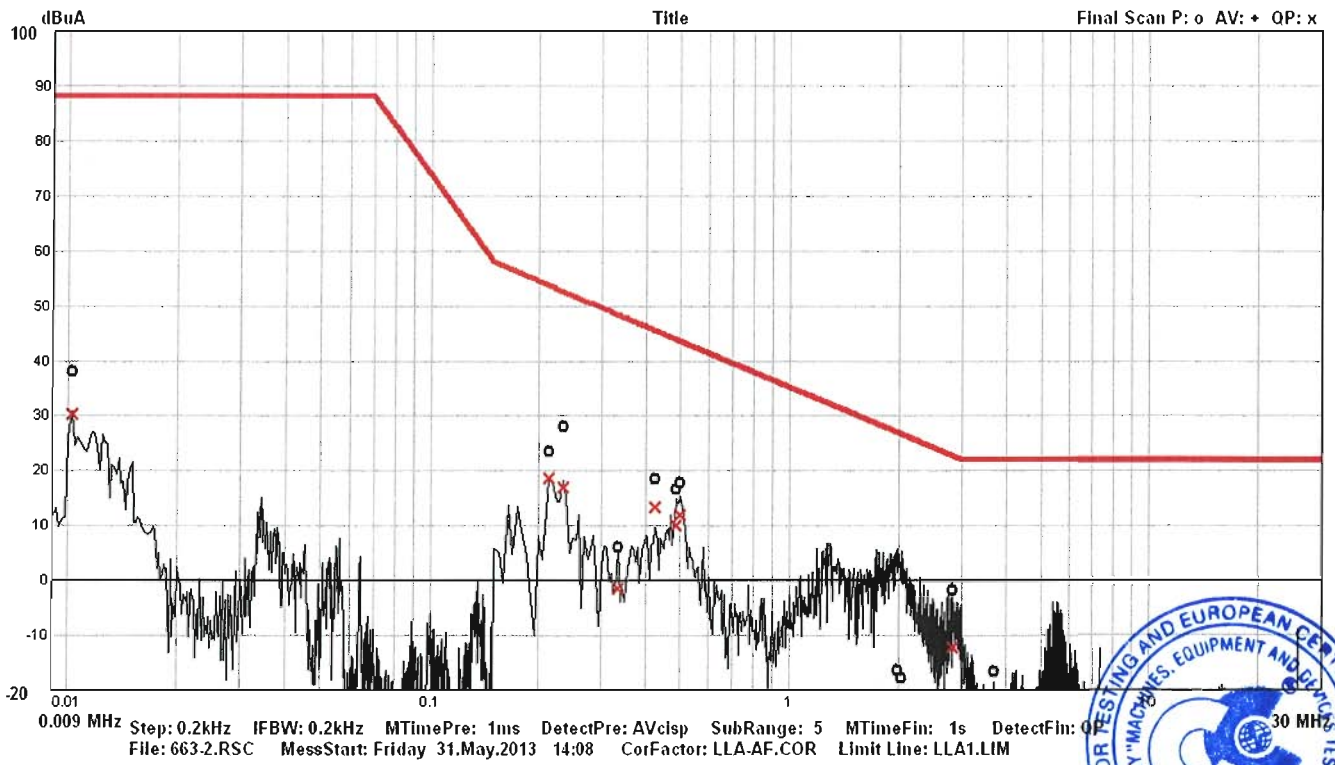

*The results showed in present test report concern tested sample only
The test report could be reproduced as a whole only and after written permission of the laboratory*




Radiated electromagnetic disturbances - measured along the axis - Z

Frequency

Quasi peak - QP

	Measuring	Margin	Measuring
MHz	dB(μA)	dB(μA)	dB(μA)
0,011	27,55	60,45	88,00
0,215	17,79	35,88	53,67
0,230	17,98	34,88	52,86
0,295	1,88	47,99	49,87
0,380	6,66	40,16	46,82
0,490	8,32	35,45	43,77
0,500	7,90	35,63	43,53
1,375	-14,25	45,62	31,37
1,710	-8,99	37,74	28,75
2,180	-18,99	44,82	25,83
2,760	-29,15	52,15	23,00
3,010	-29,59	51,59	22,00
3,520	-34,18	56,18	22,00
4,270	-36,81	58,81	22,00
7,345	-31,93	53,93	22,00
30,000	-23,31	45,31	22,00

Drawing of Radiated electromagnetic disturbances - measured along the axis - Z

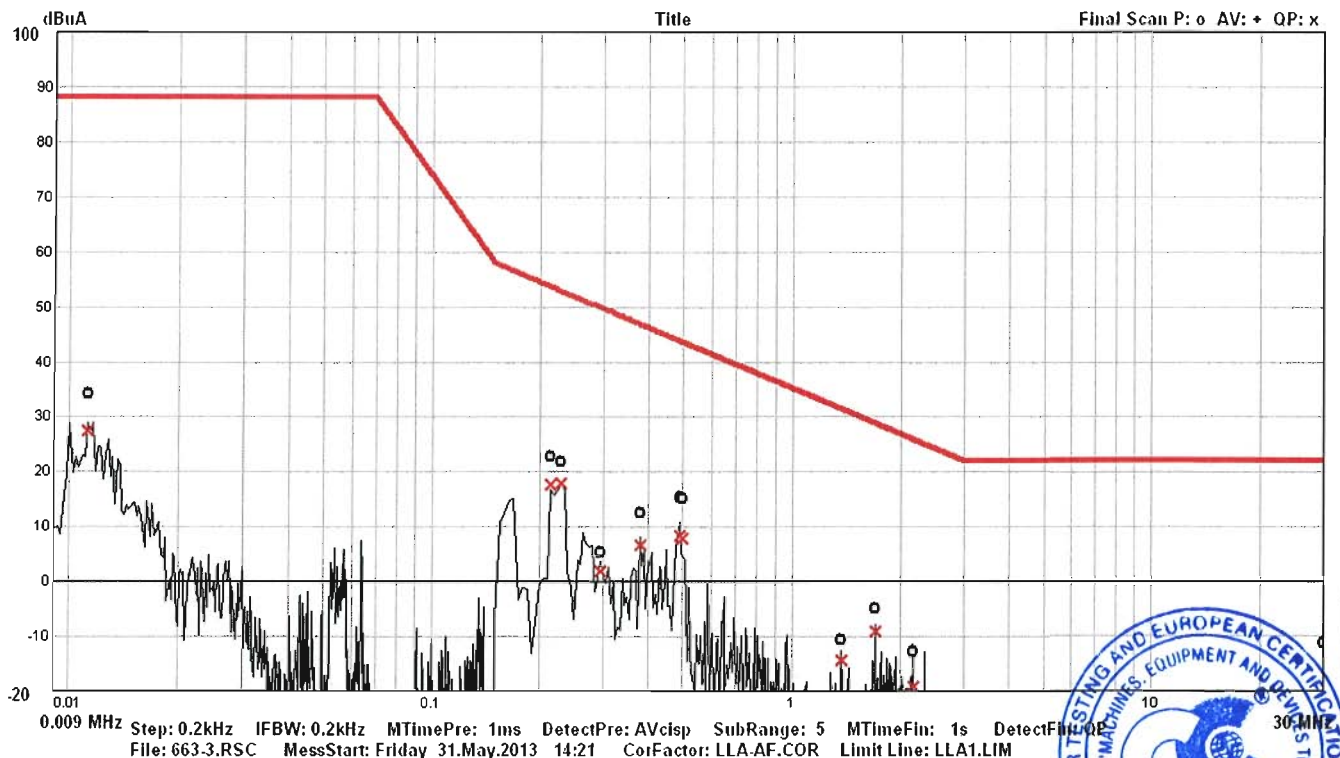

*The results showed in present test report concern tested sample only
The test report could be reproduced as a whole only and after written permission of the laboratory*

2. Radiated electromagnetic disturbances – 30MHz ÷ 300MHz

EN 55015, cl. 4.4.2 – Frequency range 30MHz to 300MHz – Annex B. Limits - Table B.1

EN 55015, cl. 5.2.4 – Other luminaires

EN 55015, cl. 6 – Operating conditions for lighting equipment


EN 55015, cl. 6.4 – Ambient temperature: 25 °C ; Relative Humidity: 42 %.

EN 55015, cl.9.2 – Measuring arrangement and procedure related to Subclause 4.4.2

RESULTS OF MEASUREMENT :

Frequency	Radiated electromagnetic disturbances		
	Quasi peak - QP		
	Measuring	Margin	Measuring
MHz	dB(μV)	dB(μV)	dB(μV)
42,10	28,93	32,25	61,18
65,20	23,44	34,11	57,55
98,30	48,81	5,33	54,14
135,20	30,33	23,67	54,00
153,40	13,07	40,93	54,00
191,30	35,96	18,04	54,00
197,80	27,85	26,15	54,00
229,20	13,20	40,80	54,00
253,20	13,17	47,83	61,00
275,30	13,06	47,94	61,00

Drawing of Radiated electromagnetic disturbances

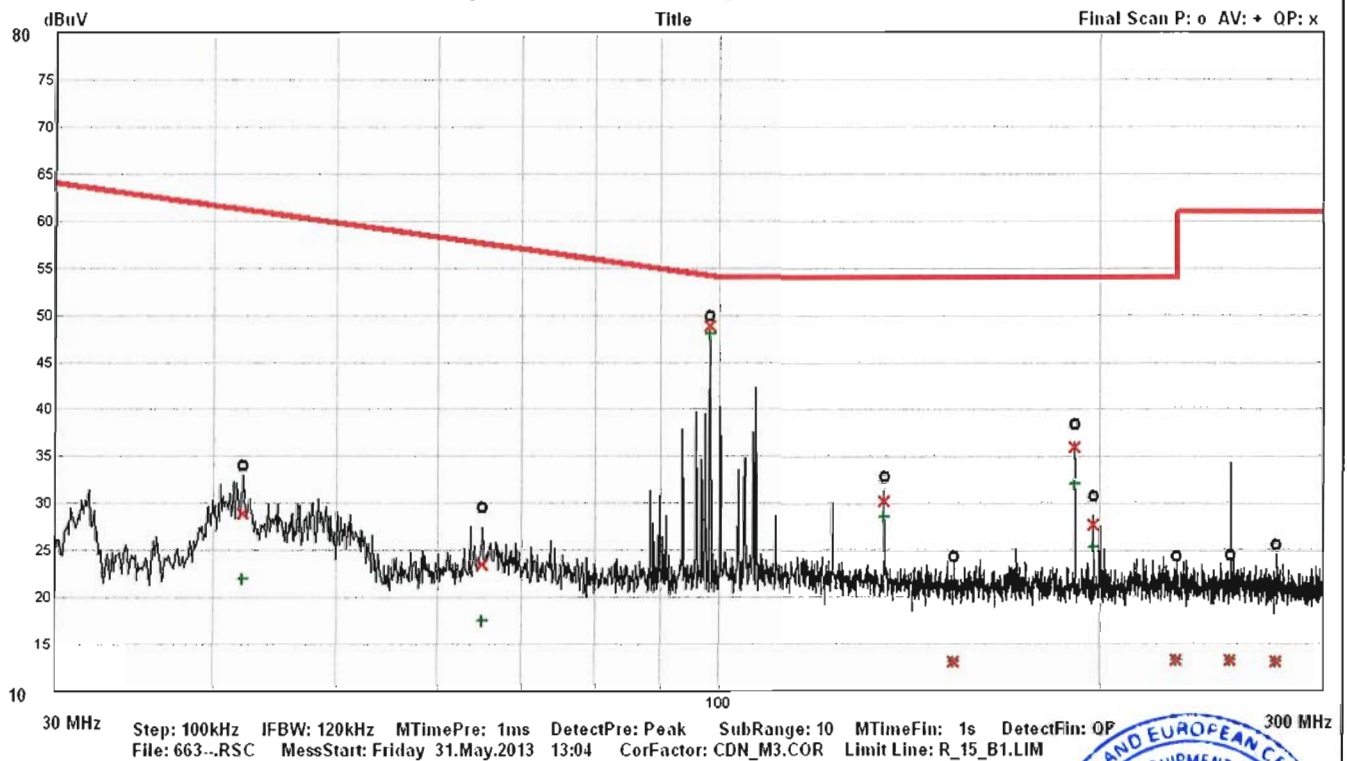

The results showed in present test report concern tested sample only
The test report could be reproduced as a whole only and after written permission of the laboratory






3. HARMONIC CURRENT MEASUREMENT

Classification of equipment - C

Duration of test - 2.5 min

THC= 0,3679 A I-THD= 18,881 % POHC= 0,01474 A POHC Limit= 0,18893 A

V_{RMS} = 229,9 V I_{peak} = 3,426 A Frequency = 50 Hz

I_{RMS} = 2,027 A I_F = 1,992 A Power= 453,4 W

Crest Factor= 1,69 Power Factor = 0,97 K Factor= 1,898

Harmonic	AVERAGE VALUES			MAX VALUE		
	Measured	100% Limit	% of Limit	Measured	150% Limit	% of Limit
№	, A	, A	%	, A	, A	%
2	0,0023	0,0398	6	0,0028	0,0598	5
3	0,3297	0,5795	57	0,3307	0,8699	38
5	0,1133	0,1992	57	0,1141	0,2990	38
7	0,0555	0,1394	40	0,0561	0,2093	27
9	0,0653	0,0996	66	0,0662	0,1495	44
11	0,0537	0,0597	90	0,0550	0,0897	61
13	0,0527	0,0597	88	0,0540	0,0897	60
15	0,0082	0,0597	14	0,0100	0,0897	11
17	0,0176	0,0597	30	0,0189	0,0897	21
19	0,0125	0,0597	21	0,0129	0,0897	14
21	0,0057	0,0597	10	0,0060	0,0897	7
23	0,0036	0,0597	6	0,0038	0,0897	4
25	0,0076	0,0597	13	0,0078	0,0897	9
27	0,0017	0,0597	3	0,0018	0,0897	2
29	0,0036	0,0597	6	0,0036	0,0897	4
31	0,0090	0,0597	15	0,0090	0,0897	10
33	0,0024	0,0597	4	0,0026	0,0897	3
35	0,0010	0,0597	2	0,0010	0,0897	1
37	0,0014	0,0597	2	0,0016	0,0897	2
39	0,0031	0,0597	5	0,0032	0,0897	4

*The results showed in present test report concern tested sample only
The test report could be reproduced as a whole only and after written permission of the laboratory*



Handwritten signature/initials.



Harmonics of power supply source

$V_{RMS} = 229,9 \text{ V}$

$I_{peak} = 3,426 \text{ A}$

Frequency = 50 Hz

$I_{RMS} = 2,027 \text{ A}$

$I_F = 1,992 \text{ A}$

Power = 453,4 W

Power Factor = 0,97

Harmonic	Measured	100% Limit	% of Limit
№	V	V	%
2	0,0940	0,460	20,4
3	0,9806	2,069	47,4
4	0,3381	0,460	73,5
5	0,8600	0,920	93,5
6	0,2529	0,460	55,0
7	0,2753	0,690	39,9
8	0,2301	0,460	50,0
9	0,4385	0,460	95,4
10	0,2072	0,460	45,1
11	0,2050	0,230	89,2
12	0,2144	0,230	93,3
13	0,2076	0,230	90,3
14	0,1168	0,230	50,8
15	0,0418	0,230	18,2
16	0,0697	0,230	30,3
17	0,0690	0,230	30,0
18	0,0460	0,230	20,0
19	0,0464	0,230	20,2
20	0,0463	0,230	20,1
21	0,1140	0,230	49,6
22	0,0233	0,230	10,1
23	0,0241	0,230	10,5
24	0,0230	0,230	10,0
25	0,0234	0,230	10,2
26	0,0230	0,230	10,0
27	0,0230	0,230	10,0
28	0,0230	0,230	10,0
29	0,0230	0,230	10,0
30	0,0230	0,230	10,0
31	0,0230	0,230	10,0
32	0,0230	0,230	10,0
33	0,0115	0,230	5,0
34	0,0093	0,230	4,1
35	0,0003	0,230	0,1
36	0,0225	0,230	9,8
37	0,0227	0,230	9,9
38	0,0005	0,230	0,2
39	0,0228	0,230	9,9
40	0,0193	0,230	8,4


The results showed in present test report concern tested sample only

The test report could be reproduced as a whole only and after written permission of the laboratory




M/V

Current and voltage waveform

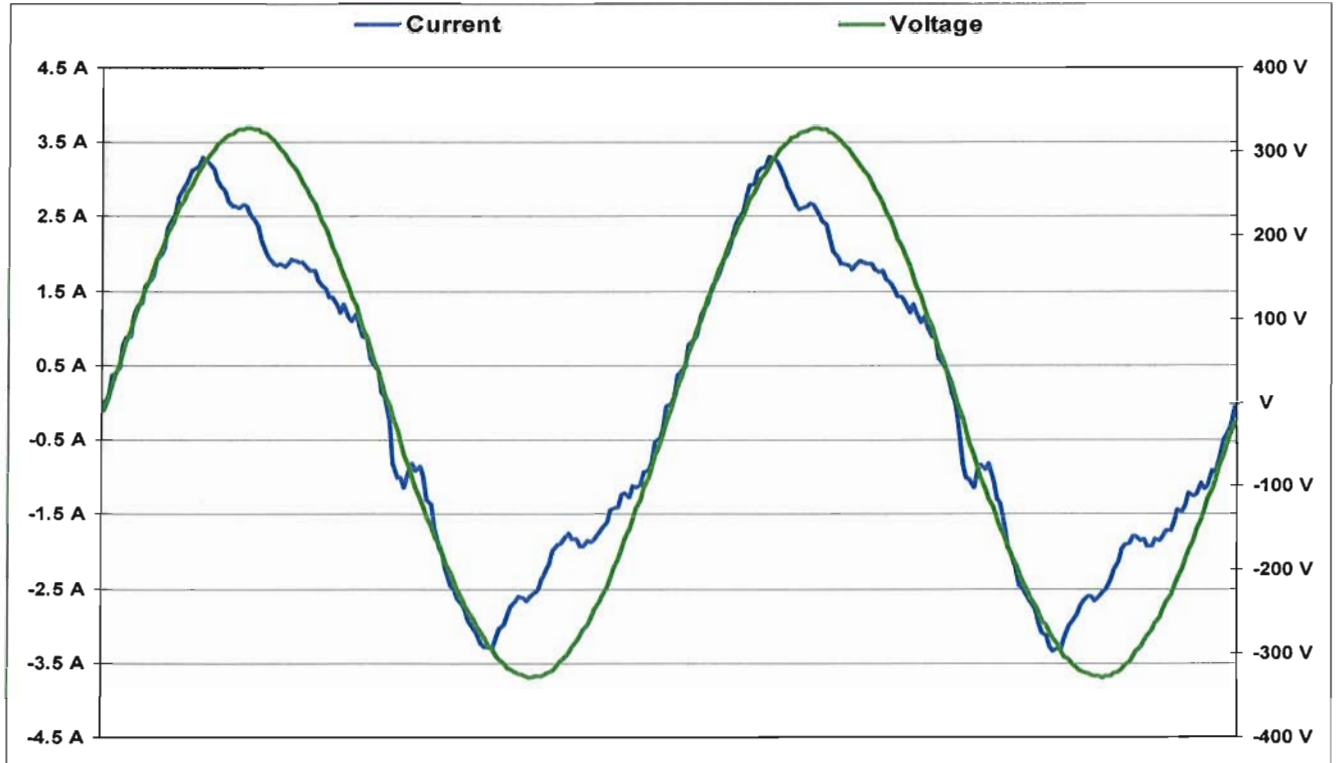

Graphics harmonics

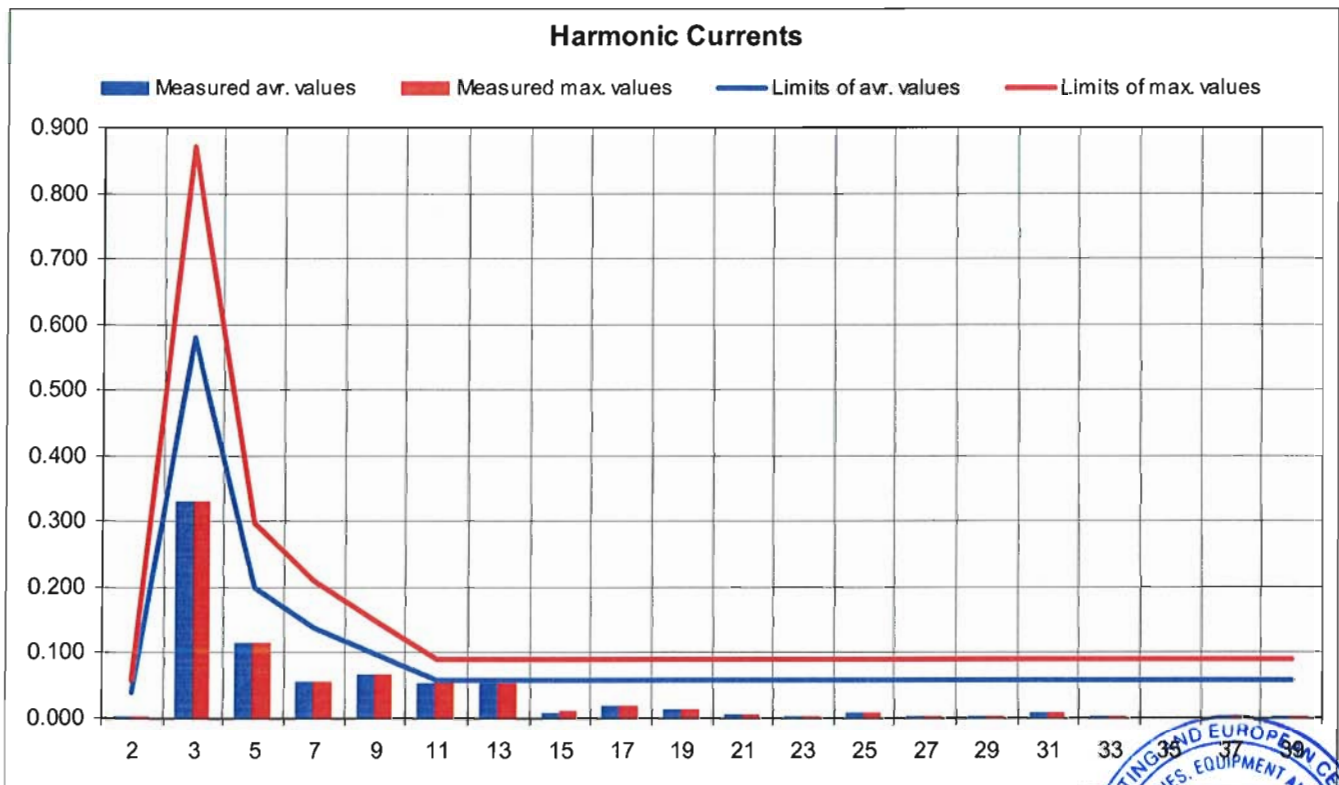

The results showed in present test report concern tested sample only
The test report could be reproduced as a whole only and after written permission of the laboratory



[Handwritten signature]



4. Voltage fluctuations and flicker measurement

EN 61000-3-3, cl. 4 – Assessment of voltage changes, voltage fluctuations and flicker

EN 61000-3-3, cl. 5 – Limits

EN 61000-3-3, cl. 6 – Test conditions

EN 61000-3-3, cl. 6.5 - Observation period

According to EN 61000-3-3:2008 – Annex A, clause A.2 luminaire is deemed to satisfy the requirements of the standard without testing of the EUT



II. Immunity of Radio disturbance characteristics for general lighting purposes

EN 61547 cl. 4.2 – Performance criteria for lighting equipment

Performance criterion A

During the test, no change of the luminous intensity shall be observed and the regulating control, if any, shall operate during the test as intended.

Performance criterion B

During the test, the luminous intensity may change to any value. After the test, the luminous intensity shall be restored to its initial value within 1 min. Regulating controls need not function during the test, but after the test, the mode of the control shall be the same as before the test provided that during the test no mode changing commands were given.

Performance criterion C

During and after the test, any change of the luminous intensity is allowed and the lamp(s) may be extinguished. After the test, within 30 min, all functions shall return to normal, if necessary by temporary interruption of the mains supply and/or operating the regulating control.

Additional requirement for lighting equipment incorporating a starting device: After the test, the lighting equipment is switched off. After half an hour, it is switched on again. The lighting equipment shall start and operate as intended.

Environment requirements during the test	Ambient temperature	15 to 35 °C
	Relative Humidity	30 to 60 %
	Air pressure	860 to 1060 mbar
Test environment	Ambient temperature	25 °C
	Relative Humidity	42 %
	Air pressure	1010 mbar

*The results showed in present test report concern tested sample only
The test report could be reproduced as a whole only and after written permission of the laboratory*




1. IMMUNITY TO ELECTROSTATIC DISCHARGE (ESD)

EN 61547, т. 5.2 – Electrostatic discharges – Table 1 - Test levels at enclosure port
 EN 61000-4-2, т. 7 – Test setup
 EN 61000-4-2, т. 7.2.2 – Table-top equipment , Figure 4
 EN 61000-4-2, т. 8 – Test procedure

Time interval between discharges	1 s
Discharge impedance	150 pF
Discharge impedance	330 Ω
Performance Criteria according cl.6.3.4 and Table 15 of EN 61547	Criteria B
Number of discharges	10 positive and 10 negative at the selected points

Discharge location	Type of discharge	Level	Test voltage	Polarity	Result
Glass - O	Air - Direct	3	8 kV	+ -	Pass (criteria A)
Body of luminaire – X	Contact - Direct	2	4 kV	+ -	Pass (criteria A)
Vertical coupling plane (VCP) – X	Contact - Direct	2	4 kV	+ -	Pass (criteria A)
Horizontal coupling plane (HCP) – X	Contact - Direct	2	4 kV	+ -	Pass (criteria A)

Picture of the object with marked points of discharge locations

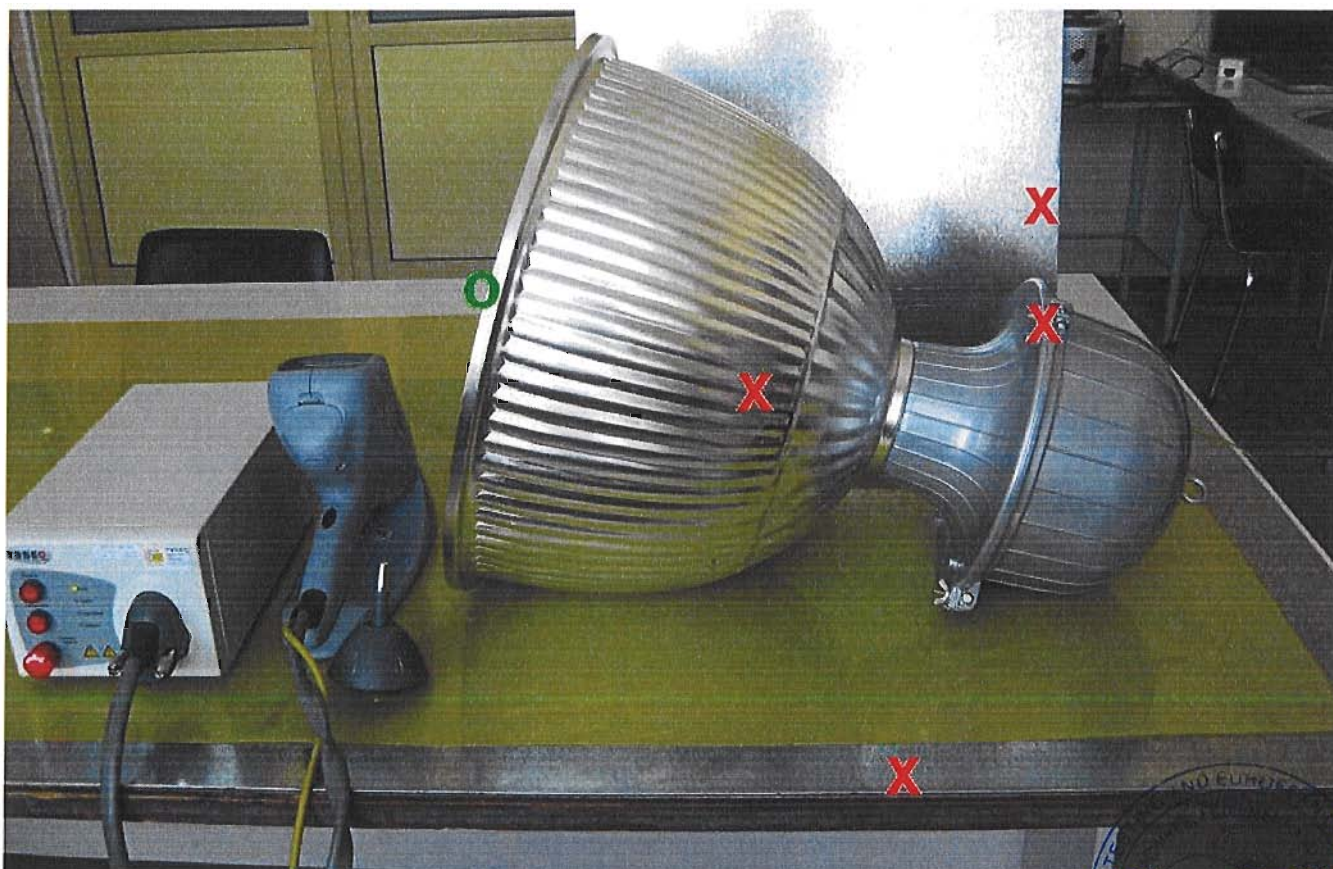

*The results showed in present test report concern tested sample only
 The test report could be reproduced as a whole only and after written permission of the laboratory*



2. ELECTRICAL FAST TRANSIENT/BURST IMMUNITY TEST

EN 61547, т. 5.5 – Applicability, Table 6

EN 61000-4-4, т. 7 – Test setup

EN 61000-4-4, т. 8 – Test procedure

Rise time	5 ns ± 30 %
Duration	50 ns ± 30 %
Repetition frequency	5 kHz
Burst duration	15 ms ± 20 % за 5 kHz
Burst period	300 ms ± 20 %
Time of application	1 min for each polarity and coupling
Performance Criteria according to cl.6.3.4 and Table 15 of EN 61547	Criteria B

Pulse Application	Application	Level	Test Voltage V	Polarity	Result
Between L and Ground plane	Coupling network	1	500	+	Pass (criteria B)
				-	Pass (criteria B)
		2	1000	+	Pass (criteria B)
				-	Pass (criteria B)
Between neutral and Ground plane	Coupling network	1	500	+	Pass (criteria B)
				-	Pass (criteria B)
		2	1000	+	Pass (criteria B)
				-	Pass (criteria B)
Between PE and Ground plane	Coupling network	1	500	+	Pass (criteria B)
				-	Pass (criteria B)
		2	1000	+	Pass (criteria B)
				-	Pass (criteria B)
Between L, neutral, PE and Ground plane	Coupling network	1	500	+	Pass (criteria B)
				-	Pass (criteria B)
		2	1000	+	Pass (criteria B)
				-	Pass (criteria B)

Signal lines

Pulse Application	Application	Level	Test Voltage V	Polarity	Result
-	Coupling clamp	1	500	+	-
				-	-
-	Coupling clamp	2	1000	+	-
				-	-

Control lines

Pulse Application	Application	Level	Test Voltage V	Polarity	Result
-	Coupling clamp	1	500	+	-
				-	-
-	Coupling clamp	2	1000	+	-
				-	-

*The results showed in present test report concern tested sample only
The test report could be reproduced as a whole only and after written permission of the laboratory*





3. SURGE IMMUNITY TEST

EN 61547, τ. 5.7 – Applicability ,Table 10
EN 61000-4-5, τ. 7 – Test setup
EN 61000-4-2, τ. 8 – Test procedure

Front time	1,2 μs ± 30 %		
Time to half value	50 μs ± 20 %		
Source impedance	Power line symmetrical	2 Ω + 18 μF	
	Power line unsymmetrical	12 Ω + 9 μF	
Phase angles	90°/ 270°		
Number of surges / polarity /phase angle	5		
Performance Criteria according to cl.6.3.4 and Table 15 of EN 61547	Criteria C		

Power line symmetrical

Pulse Application	Level	Test Voltage V	Polarity	Result
phase L – neutral N	1	500	+	Pass (criteria B)
			-	Pass (criteria B)
	2	1000	+	Pass (criteria B)
			-	Pass (criteria B)

Power line unsymmetrical

Pulse Application	Level	Test Voltage V	Polarity	Result
phase L – protective earth	1	500	+	Pass (criteria A)
			-	Pass (criteria A)
	2	1000	+	Pass (criteria A)
			-	Pass (criteria A)
	3	2000	+	Pass (criteria A)
			-	Pass (criteria A)
neutral N – protective earth	1	500	+	Pass (criteria A)
			-	Pass (criteria A)
	2	1000	+	Pass (criteria A)
			-	Pass (criteria A)
	3	2000	+	Pass (criteria A)
			-	Pass (criteria A)

*The results showed in present test report concern tested sample only
The test report could be reproduced as a whole only and after written permission of the laboratory*





4. RATED POWER FREQUENCY MAGNETIC FIELD

EN 61547, τ. 5.4 – Applicability ,Table 3

EN 61000-4-8 τ. 7 – Test setup

EN 61000-4-8 τ. 8 – Test procedure

Performance Criteria according to cl.6.3.3
and Table 15 of EN 61547

Criteria A

Standard inductive coil	Orientation of standard inductive coil	Level	Field strength in the centre for all other inductive coils	Current in the coil (a coil with 10 windings)	Result
1 m x 1 m	X	2	3 A/m	3,45 A	Pass (criteria A)
1 m x 1 m	Y	2	3 A/m	3,45 A	Pass (criteria A)
1 m x 1 m	Z	2	3 A/m	3,45 A	Pass (criteria A)

*The results showed in present test report concern tested sample only
The test report could be reproduced as a whole only and after written permission of the laboratory*





5. Voltage dips, short interruptions and voltage variations immunity tests

5.1 Voltage dips immunity tests

EN 61547, τ. 5.8 – Applicability ,Table 11

EN 61000-4-11 τ. 7 – Test setup

EN 61000-4-11 τ. 8 – Test procedure

EN 61000-4-11 τ. 8.2.1 – Testing for each selected combination of test level and duration with a sequence of three dips with intervals of 10 s minimum (between each test event)

Performance Criteria according to cl.6.3.4 and Table 15 of EN 61547

Criteria C

Voltage test levels (% of rated voltage)	Duration (cycles)	Phase angle synchronization	Result
70 %	10 cycles	0°	Pass (criteria C)

5.2 Short interruptions immunity tests

EN 61547, τ. 5.8 – Applicability ,Table 12

EN 61000-4-11 τ. 7 – Test setup

EN 61000-4-11 τ. 8 – Test procedure

EN 61000-4-11 τ. 8.2.1 – Testing for each selected combination of test level and duration with a sequence of three interruptions with intervals of 10 s minimum (between each test event)

Performance Criteria according to cl.6.3.4 and Table 15 of EN 61547

Criteria B

Voltage test levels (% of rated voltage)	Duration (cycles)	Phase angle synchronization	Result
0 %	0,5 cycles	0°	Pass (criteria B)

*The results showed in present test report concern tested sample only
The test report could be reproduced as a whole only and after written permission of the laboratory*





USED TECHNICAL EQUIPMENTS:

	Appliance	Type	Manufacturer	Identity №	Last calibration date
1.	ESD - Generator	NSG438	TESEQ Switzerland	988	14.03.2012
2.	EFT/B - Generator	NSG 2050 INA 2050 PNW 2225 CDN 133	Schaffner Electrotest GmbH, Germany	200902-653LU 200906-578LU 200838-570LU 34460	14.03.2012
3.	Surge - Generator	NSG 2050 INA 2050 PNW 2050 CDN 133	Schaffner Electrotest GmbH, Germany	200902-653LU 200906-578LU 200911-636LU 34460	16.03.2012
4.	Digital multimeter	UNIGOR 390	LEM Austria	PI 3288	08.07.2011
5.	Voltage Generator	GL 01-16-230	Neosvet Bulgaria	0001	-
6.	Power Quality Analyzer	435	Fluke Netherlands	DM 9881064	08.11.2011
7.	Thermometer-higrometer	177-H1	TESTO Germany	01320300/902	19.04.2012
8.	EMI – receiver 9 kHz ÷ 1000 MHz	SCR 3501	Schaffner Electrotest GmbH, Germany	522	07.07.2011
9.	Large loop antenna 2m	RF300	Laplace Instruments LTD U.K.	9123	12.03.2013
10.	Coupling/Decoupling network	CDN M2+M3	Frankonia EMC Test - Systems	A2210229	18.04.2013

TEST PERFORMER: 1.

/ T. Hristov

2.

/D. Chavalinov/

CHIEF LABORATORY :

/ T. Hristov /

