



**LABORATORY FOR TESTING OF MACHINERY,
EQUIPMENT AND DEVICES**
CENTER FOR TESTING AND EUROPEAN CERTIFICATION LTD

2, Industrialna Str., Stara Zagora, Bulgaria,
Tel.: +359 42 620 368 Fax: +359 42 602 377 ctec@ctec-sz.com

TEST REPORT

№ 2emc-i-14-905/20.06.2014

OBJECT TO BE TESTED: Luminaire "GALA" 4x18W/T8 with cat. № 9GOME418
Representative sample from fixtures group "GALA" with cat. №: 9GOME218; 9GOME418
*(name of object to be tested, type, model, quantity,
type – portable, fixed, for walling in and other)*

APPLICANT FOR TEST: "ELMARK INDUSTRIES" SC. 2 Dobrudja Blvd. Dobrich, Bulgaria ,
Tel.: 058 500 055, e-mail: denkov@elmark.bg
Application № 905/ 14.03.2014
(name of the firm – applicant, address, telephone, number and date of the test application)

STANDARD:

- BDS EN 55015:2006+A1:2007+A2:2009 Limits and methods of measurement of radio disturbance characteristics of electrical lighting and similar equipment.
BDS EN 61000-3-2:2006+A1:2009+A2:2009 Electromagnetic compatibility (EMC).
Part 3-2: Limits – Limits for harmonic current emissions (equipment input current ≤ 16 A per phase).
BDS EN 61000-3-3:2008 Electromagnetic compatibility (EMC).
Part 3-3: Limits - Limitation of voltage changes, voltage fluctuations and flicker in public low-voltage supply systems, for equipment with rated current ≤ 16 A per phase and not subject to conditional connection.
BDS EN 61547:2009 Equipment for general lighting purposes - EMC immunity requirements
BDS EN 61000-4-2:2009 Electromagnetic compatibility (EMC).
Part 4-2: Testing and measurement techniques - Electrostatic discharge immunity test
BDS EN 61000-4-4:2004+A1:2010 Electromagnetic compatibility (EMC).
Part 4-4: Testing and measurement techniques - Electrical fast transient/burst immunity test
BDS EN 61000-4-5:2006 Electromagnetic compatibility (EMC).
Part 4-5: Testing and measurement techniques - Surge immunity test
BDS EN 61000-4-8:2010 Electromagnetic compatibility (EMC).
Part 4-8: Testing and measurement techniques - Power frequency magnetic field immunity test
BDS EN 61000-4-11:2004 Electromagnetic compatibility (EMC).
Part 4-11: Testing and measurement techniques – Voltage dips, short interruptions and voltage variations immunity tests
(number and name of the standards)

DATE OF ACCEPTANCE IN THE TEST LABORATORY: 21.03.2014

YEAR OF PRODUCTION : 2014
(identification number)

MANUFACTURER: "ELMARK INDUSTRIES" SC. 2 Dobrudja Blvd. Dobrich, Bulgaria ,
Tel.: 058 500 055, e-mail: denkov@elmark.bg
(firm, trade mark, address)

DECLARED TECHNICAL DATA: Rated voltage – 230 V AC
Rated frequency – 50 Hz
Rated power – 4x18 W
Class I

DATE OF TEST PERFORMANCE: 30.05.2014 - 17.06.2014

LABORATORY CHIEF:
/ T. Hristov /



*The results showed in present test report concern tested sample only
The test report could be reproduced as a whole only and after written permission of the laboratory*

Page 1 of 16



I. Emission of Radio disturbance characteristics of electrical lighting and similar equipment


1. Radiated electromagnetic disturbances – 9kHz ÷ 30MHz

BDS EN 55015, cl. 4.4 – Radiated electromagnetic disturbances, limits – Table 3
 BDS EN 55015, cl. 5.2.4 – Other luminaires
 BDS EN 55015, cl. 6 – Operating conditions for lighting equipment
 BDS EN 55015, cl. 6.4 – Ambient temperature: 24 °C ; Relative Humidity: 44 %
 BDS EN 55015, cl.9.1 – Measuring arrangement and procedure
 BDS EN 55015, cl.9.2 – Indoor and outdoor luminaires
 The test is performed at supply voltage: 230 V

RESULTS OF MEASUREMENT :

| Frequency MHz | Radiated electromagnetic disturbances - measured along the axis - X | | |
|------------------|---|------------------|-----------------|
| | Quasi peak - QP | | |
| | Measuring dB(μA) | Margin dB(μA) | Limit dB(μA) |
| 0,037 | 11,97 | 76,03 | 88,00 |
| 0,038 | 39,74 | 48,26 | 88,00 |
| 0,114 | 14,33 | 54,47 | 68,80 |
| 0,190 | 21,87 | 33,28 | 55,15 |
| 0,285 | 14,69 | 35,59 | 50,28 |
| 0,345 | 12,72 | 35,27 | 47,99 |
| 0,370 | 11,14 | 36,01 | 47,15 |
| 0,495 | 7,30 | 36,35 | 43,65 |
| 0,500 | 5,95 | 37,58 | 43,53 |
| 1,490 | 4,87 | 25,53 | 30,40 |
| 1,595 | 8,52 | 21,07 | 29,59 |
| 2,345 | 4,68 | 20,28 | 24,96 |
| 2,965 | -2,27 | 24,41 | 22,14 |
| 3,010 | -2,50 | 24,50 | 22,00 |
| 4,580 | -21,85 | 43,85 | 22,00 |
| 4,815 | -18,85 | 40,85 | 22,00 |

Drawing of Radiated electromagnetic disturbances - measured along the axis - X

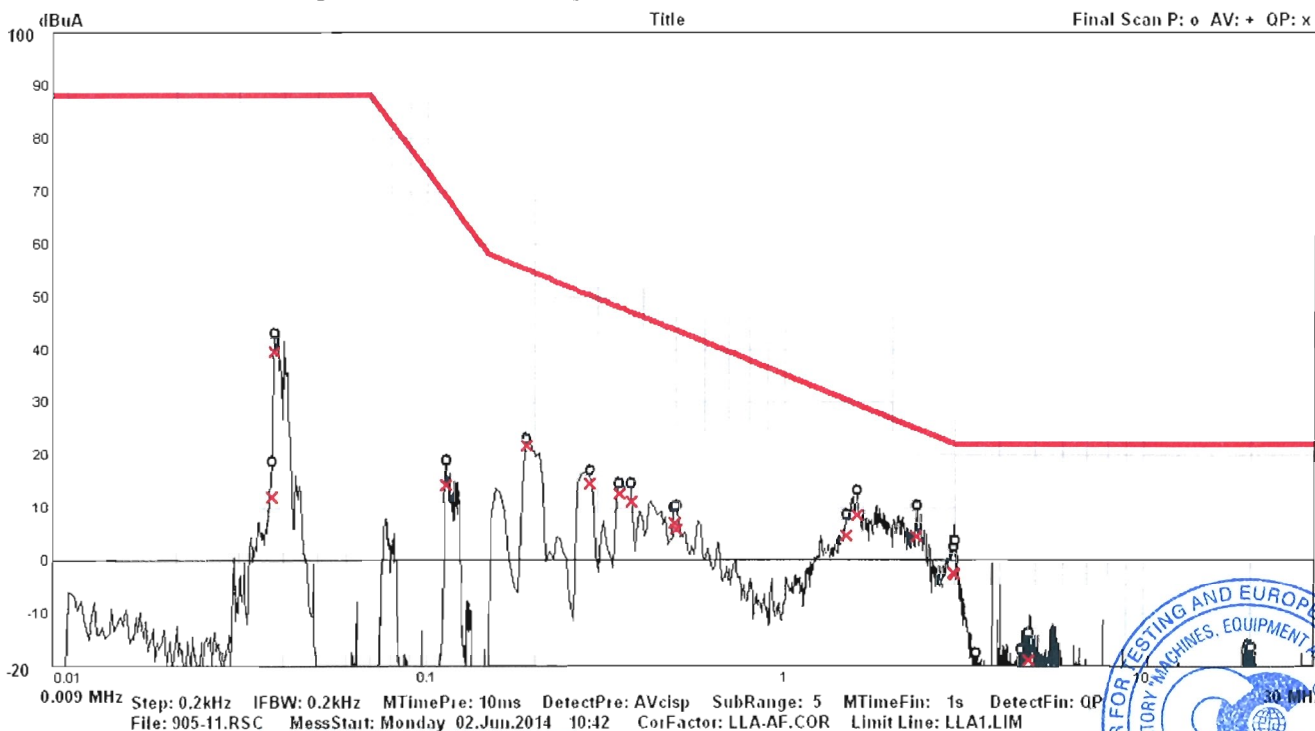

*The results showed in present test report concern tested sample only
 The test report could be reproduced as a whole only and after written permission of the laboratory*






Radiated electromagnetic disturbances - measured along the axis - Y

Frequency

Quasi peak - QP

| | Measuring | Margin | Measuring |
|------------|------------------|---------------|------------------|
| MHz | dB(μA) | dB(μA) | dB(μA) |
| 0,038 | 41,42 | 46,58 | 88,00 |
| 0,115 | 14,36 | 54,03 | 68,39 |
| 0,195 | 23,46 | 31,38 | 54,84 |
| 0,280 | 15,27 | 35,22 | 50,49 |
| 0,355 | 14,41 | 33,23 | 47,64 |
| 0,360 | 13,66 | 33,81 | 47,47 |
| 0,430 | 10,08 | 35,26 | 45,34 |
| 0,505 | 7,37 | 36,04 | 43,41 |
| 1,495 | 6,17 | 24,19 | 30,36 |
| 1,585 | 7,95 | 21,71 | 29,66 |
| 2,100 | 2,88 | 23,40 | 26,28 |
| 2,930 | -8,18 | 30,46 | 22,28 |
| 3,015 | -10,98 | 32,98 | 22,00 |
| 4,170 | -22,72 | 44,72 | 22,00 |
| 4,215 | -24,37 | 46,37 | 22,00 |
| 19,985 | -25,43 | 47,43 | 22,00 |

Drawing of Radiated electromagnetic disturbances - measured along the axis - Y

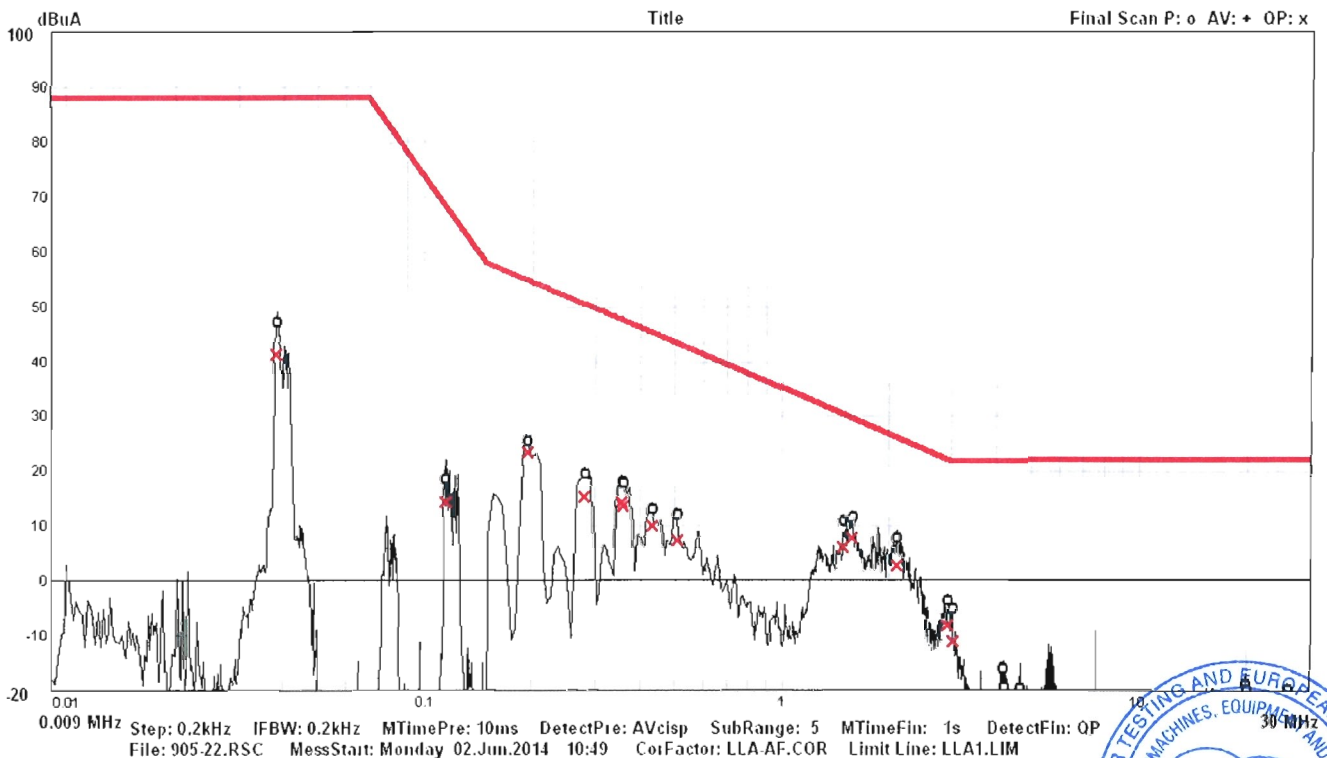


*The results showed in present test report concern tested sample only
The test report could be reproduced as a whole only and after written permission of the laboratory*





| Frequency | Radiated electromagnetic disturbances - measured along the axis - Z | | |
|-----------|---|--------|-----------|
| | Quasi peak - QP | | |
| | Measuring | Margin | Measuring |
| MHz | dB(μA) | dB(μA) | dB(μA) |
| 0,038 | 29,15 | 58,85 | 88,00 |
| 0,114 | 6,11 | 62,62 | 68,73 |
| 0,195 | 12,45 | 42,39 | 54,84 |
| 0,275 | 6,85 | 43,86 | 50,71 |
| 0,355 | 4,87 | 42,77 | 47,64 |
| 0,365 | 3,22 | 44,09 | 47,31 |
| 0,430 | 0,26 | 45,08 | 45,34 |
| 0,500 | -0,89 | 44,42 | 43,53 |
| 1,205 | -12,09 | 45,05 | 32,96 |
| 1,580 | -8,86 | 38,56 | 29,70 |
| 2,145 | -11,74 | 37,77 | 26,03 |
| 2,905 | -13,34 | 35,72 | 22,38 |
| 3,010 | -20,15 | 42,15 | 22,00 |
| 4,545 | -26,23 | 48,23 | 22,00 |
| 4,820 | -24,98 | 46,98 | 22,00 |
| 30,000 | -21,97 | 43,97 | 22,00 |

Drawing of Radiated electromagnetic disturbances - measured along the axis - Z

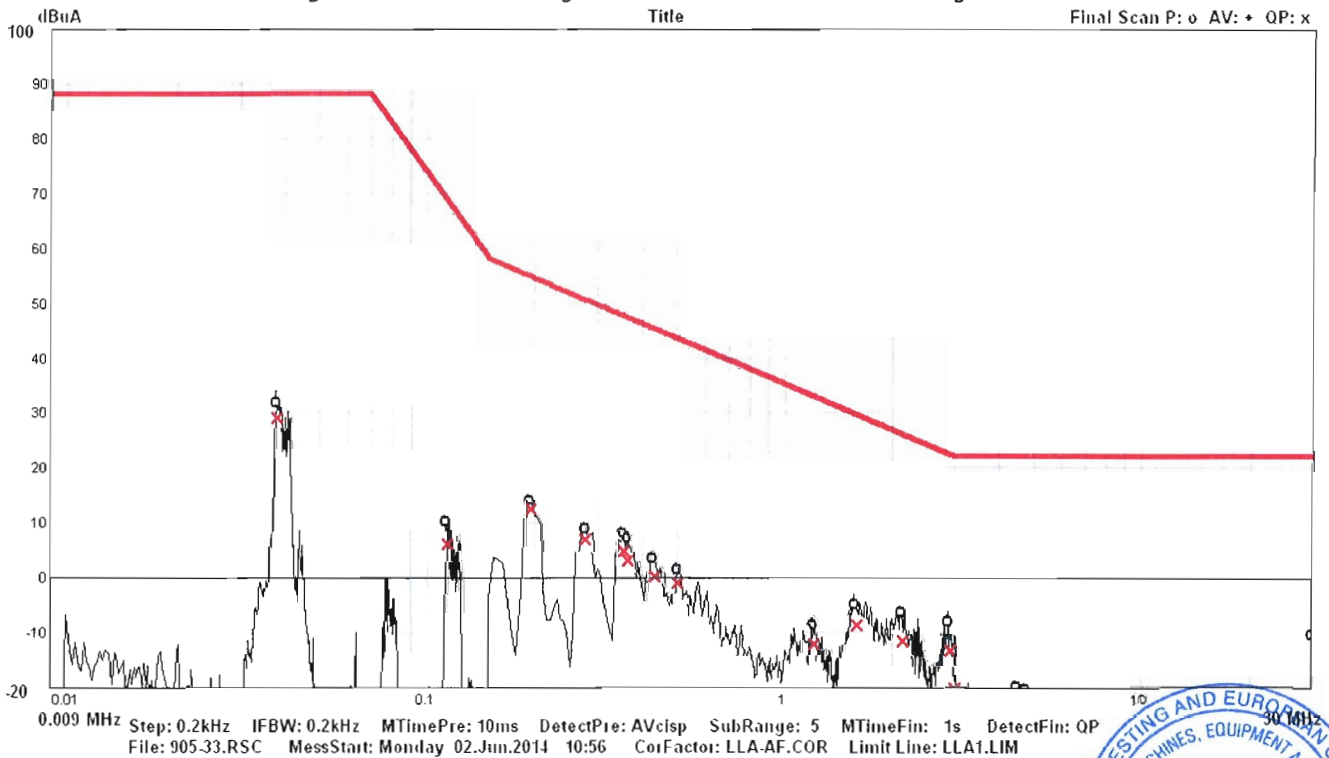

*The results showed in present test report concern tested sample only
The test report could be reproduced as a whole only and after written permission of the laboratory*






2. Radiated electromagnetic disturbances – 30MHz ÷ 300MHz
 BDS EN 55015, cl. 4.4.2 – Frequency range 30MHz to 300MHz – Annex B. Limits - Table B.1
 BDS EN 55015, cl. 5.2.4 – Other luminaires
 BDS EN 55015, cl. 6 – Operating conditions for lighting equipment
 BDS EN 55015, cl. 6.4 – Ambient temperature: 25 °C ; Relative Humidity: 46 %.
 BDS EN 55015, cl.9.2 – Measuring arrangement and procedure related to Subclause 4.4.2

RESULTS OF MEASUREMENT :

| Frequency | Radiated electromagnetic disturbances | | |
|-----------|---------------------------------------|--------|-----------|
| | Quasi peak - QP | | |
| | Measuring | Margin | Measuring |
| MHz | dB(μV) | dB(μV) | dB(μV) |
| 54,20 | 33,73 | 25,35 | 59,08 |
| 57,10 | 29,76 | 28,89 | 58,65 |
| 98,30 | 45,22 | 8,92 | 54,14 |
| 135,20 | 27,33 | 26,67 | 54,00 |
| 159,70 | 27,73 | 26,27 | 54,00 |
| 171,90 | 27,89 | 26,11 | 54,00 |
| 200,50 | 21,79 | 32,21 | 54,00 |
| 225,30 | 12,85 | 41,15 | 54,00 |
| 266,70 | 26,21 | 34,79 | 61,00 |
| 282,60 | 19,69 | 41,31 | 61,00 |

Drawing of Radiated electromagnetic disturbances

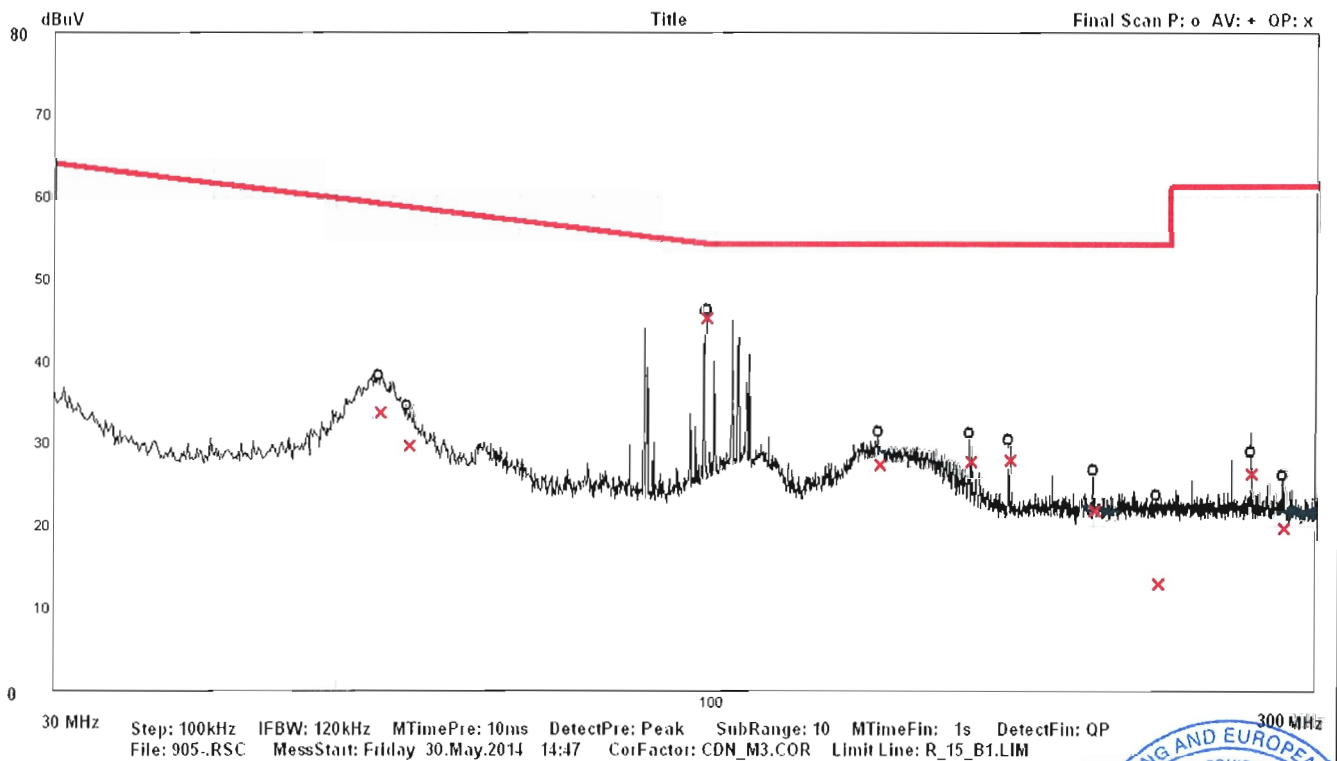

*The results showed in present test report concern tested sample only
 The test report could be reproduced as a whole only and after written permission of the laboratory*





3. HARMONIC CURRENT MEASUREMENT

Classification of equipment - C

Duration of test - 2,5 min

THC= 0,047587 A

I-THD= 15,28 %

POHC= 0,007637 A

POHC Limit= 0,029665 A

V_{RMS} = 229,7 V

I_{peak} = 0,5079 A

Frequency = 50 Hz

I_{RMS} = 0,3163 A

I_F = 0,3127 A

Power= 71,04 W

Crest Factor= 1,42

Power Factor = 0,98

K Factor= 2,01

| Harmonic | AVERAGE VALUES | | | MAX VALUE | | |
|----------|----------------|------------|------------|-----------|------------|------------|
| | Measured | 100% Limit | % of Limit | Measured | 150% Limit | % of Limit |
| № | , A | , A | % | , A | , A | % |
| 2 | 0,0007 | 0,0063 | 11 | 0,0007 | 0,0095 | 8 |
| 3 | 0,0395 | 0,0919 | 43 | 0,0402 | 0,1389 | 29 |
| 5 | 0,0191 | 0,0313 | 61 | 0,0197 | 0,0473 | 42 |
| 7 | 0,0042 | 0,0219 | 19 | 0,0051 | 0,0331 | 15 |
| 9 | 0,0114 | 0,0156 | 73 | 0,0115 | 0,0236 | 49 |
| 11 | 0,0062 | 0,0094 | 66 | 0,0068 | 0,0142 | 48 |
| 13 | 0,0082 | 0,0094 | 88 | 0,0083 | 0,0142 | 59 |
| 15 | 0,0018 | 0,0094 | 19 | 0,0021 | 0,0142 | 15 |
| 17 | 0,0049 | 0,0094 | 52 | 0,0051 | 0,0142 | 36 |
| 19 | 0,0012 | 0,0094 | 13 | 0,0016 | 0,0142 | 11 |
| 21 | 0,0045 | 0,0094 | 48 | 0,0046 | 0,0142 | 32 |
| 23 | 0,0020 | 0,0094 | 21 | 0,0022 | 0,0142 | 16 |
| 25 | 0,0037 | 0,0094 | 40 | 0,0039 | 0,0142 | 28 |
| 27 | 0,0017 | 0,0094 | 18 | 0,0020 | 0,0142 | 14 |
| 29 | 0,0024 | 0,0094 | 26 | 0,0027 | 0,0142 | 19 |
| 31 | 0,0010 | 0,0094 | 11 | 0,0013 | 0,0142 | 9 |
| 33 | 0,0019 | 0,0094 | 20 | 0,0023 | 0,0142 | 16 |
| 35 | 0,0021 | 0,0094 | 22 | 0,0023 | 0,0142 | 16 |
| 37 | 0,0012 | 0,0094 | 12 | 0,0017 | 0,0142 | 12 |
| 39 | 0,0013 | 0,0094 | 14 | 0,0015 | 0,0142 | 11 |

The results showed in present test report concern tested sample only
The test report could be reproduced as a whole only and after written permission of the laboratory





Harmonics of power supply source

$V_{RMS} = 229,7 \text{ V}$

$I_{peak} = 0,5079 \text{ A}$

Frequency = 50 Hz

$I_{RMS} = 0,3163 \text{ A}$

$I_f = 0,3127 \text{ A}$

Power = 71,04 W

Power Factor = 0,98

| Harmonic | Measured | 100% Limit | % of Limit |
|----------|----------|------------|------------|
| № | V | V | % |
| 2 | 0,1369 | 0,460 | 29,8 |
| 3 | 0,4132 | 2,069 | 20,0 |
| 4 | 0,2986 | 0,460 | 64,9 |
| 5 | 0,6404 | 0,920 | 69,6 |
| 6 | 0,1838 | 0,460 | 40,0 |
| 7 | 0,0902 | 0,690 | 13,1 |
| 8 | 0,1608 | 0,460 | 35,0 |
| 9 | 0,3675 | 0,460 | 79,9 |
| 10 | 0,1378 | 0,460 | 30,0 |
| 11 | 0,1149 | 0,230 | 50,0 |
| 12 | 0,1149 | 0,230 | 50,0 |
| 13 | 0,1150 | 0,230 | 50,0 |
| 14 | 0,0919 | 0,230 | 40,0 |
| 15 | 0,0459 | 0,230 | 20,0 |
| 16 | 0,0919 | 0,230 | 40,0 |
| 17 | 0,1150 | 0,230 | 50,0 |
| 18 | 0,0689 | 0,230 | 30,0 |
| 19 | 0,0919 | 0,230 | 40,0 |
| 20 | 0,0689 | 0,230 | 30,0 |
| 21 | 0,0453 | 0,230 | 19,7 |
| 22 | 0,0695 | 0,230 | 30,2 |
| 23 | 0,1141 | 0,230 | 49,6 |
| 24 | 0,0689 | 0,230 | 30,0 |
| 25 | 0,1518 | 0,230 | 66,0 |
| 26 | 0,0689 | 0,230 | 30,0 |
| 27 | 0,0568 | 0,230 | 24,7 |
| 28 | 0,0689 | 0,230 | 30,0 |
| 29 | 0,0230 | 0,230 | 10,0 |
| 30 | 0,0689 | 0,230 | 30,0 |
| 31 | 0,1441 | 0,230 | 62,7 |
| 32 | 0,0689 | 0,230 | 30,0 |
| 33 | 0,0230 | 0,230 | 10,0 |
| 34 | 0,0689 | 0,230 | 30,0 |
| 35 | 0,0867 | 0,230 | 37,7 |
| 36 | 0,0689 | 0,230 | 30,0 |
| 37 | 0,0230 | 0,230 | 10,0 |
| 38 | 0,0913 | 0,230 | 39,7 |
| 39 | 0,0577 | 0,230 | 25,1 |
| 40 | 0,1149 | 0,230 | 50,0 |


The results showed in present test report concern tested sample only

The test report could be reproduced as a whole only and after written permission of the laboratory






Current and voltage waveform

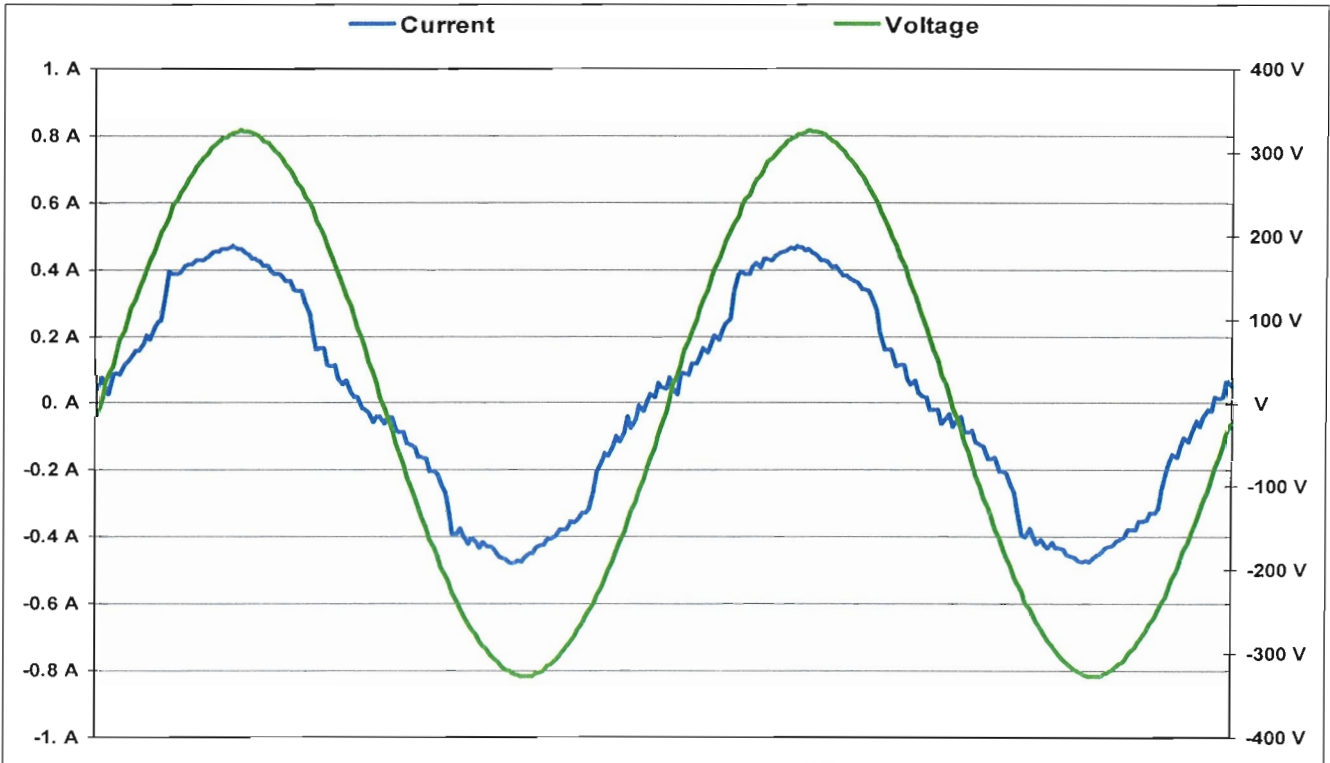

Graphics harmonics

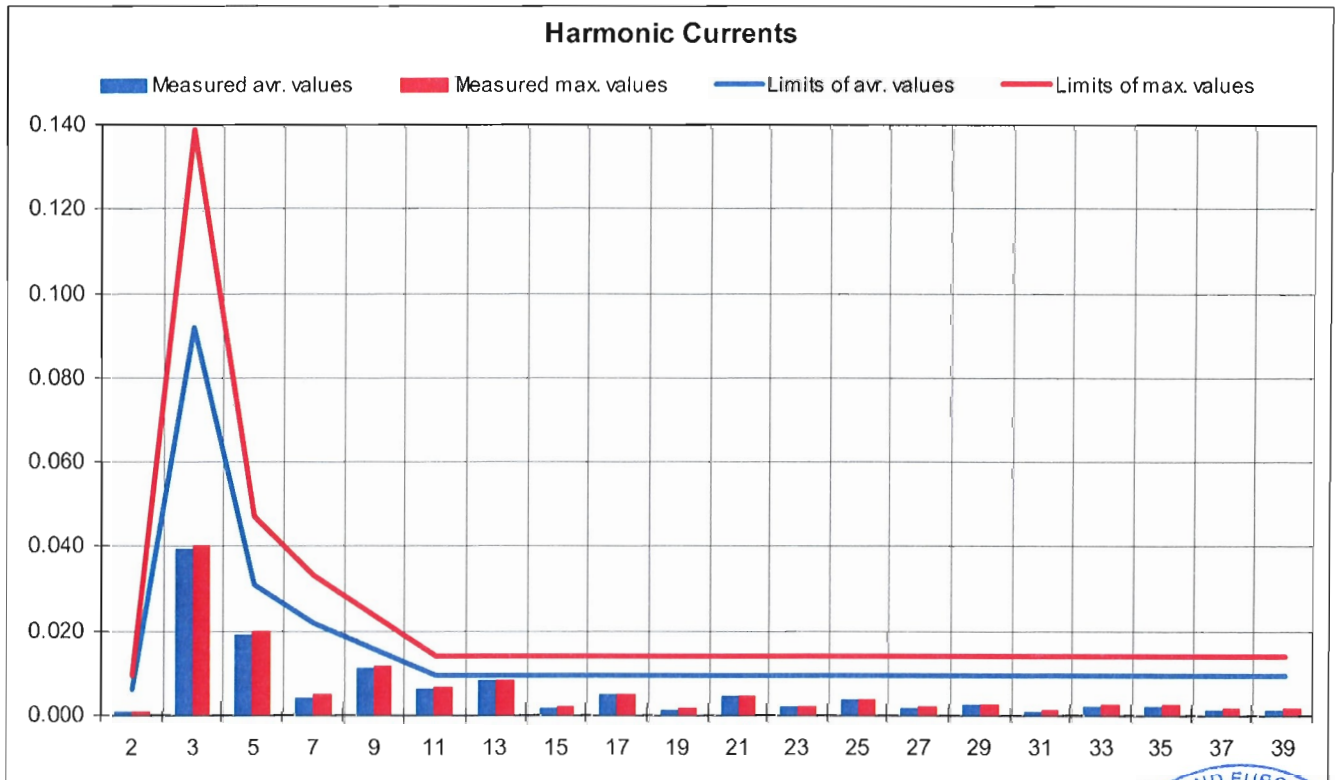

The results showed in present test report concern tested sample only
The test report could be reproduced as a whole only and after written permission of the laboratory





4. Voltage fluctuations and flicker measurement

BDS EN 61000-3-3, cl. 4 – Assessment of voltage changes, voltage fluctuations and flicker

BDS EN 61000-3-3, cl. 5 – Limits

BDS EN 61000-3-3, cl. 6 – Test conditions

BDS EN 61000-3-3, cl. 6.5 - Observation period

According to BDS EN 61000-3-3:2008 – Annex A, clause A.2 luminaire is deemed to satisfy the requirements of the standard without testing of the EUT





II. Immunity of Radio disturbance characteristics for general lighting purposes

BDS EN 61547 cl. 4.2 – Performance criteria for lighting equipment

Performance criterion A

During the test, no change of the luminous intensity shall be observed and the regulating control, if any, shall operate during the test as intended.

Performance criterion B

During the test, the luminous intensity may change to any value. After the test, the luminous intensity shall be restored to its initial value within 1 min. Regulating controls need not function during the test, but after the test, the mode of the control shall be the same as before the test provided that during the test no mode changing commands were given.

Performance criterion C

During and after the test, any change of the luminous intensity is allowed and the lamp(s) may be extinguished. After the test, within 30 min, all functions shall return to normal, if necessary by temporary interruption of the mains supply and/or operating the regulating control.

Additional requirement for lighting equipment incorporating a starting device: After the test, the lighting equipment is switched off. After half an hour, it is switched on again. The lighting equipment shall start and operate as intended.

| | | |
|--|---------------------|------------------|
| Environment requirements during the test | Ambient temperature | 15 to 35 °C |
| | Relative Humidity | 30 to 60 % |
| | Air pressure | 860 to 1060 mbar |
| Test environment | Ambient temperature | 25 °C |
| | Relative Humidity | 42 % |
| | Air pressure | 1010 mbar |

*The results showed in present test report concern tested sample only
The test report could be reproduced as a whole only and after written permission of the laboratory*




1. IMMUNITY TO ELECTROSTATIC DISCHARGE (ESD)

BDS EN 61547, τ. 5.2 – Electrostatic discharges – Table 1 - Test levels at enclosure port
 BDS EN 61000-4-2, τ. 7 – Test setup
 BDS EN 61000-4-2, τ. 7.2.2 – Table-top equipment , Figure 4
 BDS EN 61000-4-2, τ. 8 – Test procedure

| | |
|--|--|
| Time interval between discharges | 1 s |
| Discharge impedance | 150 pF |
| Discharge impedance | 330 Ω |
| Performance Criteria according cl.6.3.4 and Table 15 of BDS EN 61547 | Criteria B |
| Number of discharges | 10 positive and 10 negative at the selected points |

| Discharge location | Type of discharge | Level | Test voltage | Polarity | Result |
|--|-------------------|-------|--------------|----------|-------------------|
| Body of luminaire – X | Contact - Direct | 1;2 | 2;4 kV | + | Pass (criteria A) |
| | | | | - | |
| Vertical coupling plane (VCP) – X | Contact - Direct | 1;2 | 2;4 kV | + | Pass (criteria A) |
| | | | | - | |
| Horizontal coupling plane (HCP) – X | Contact - Direct | 1;2 | 2;4 kV | + | Pass (criteria A) |
| | | | | - | |

Picture of the object with marked points of discharge locations

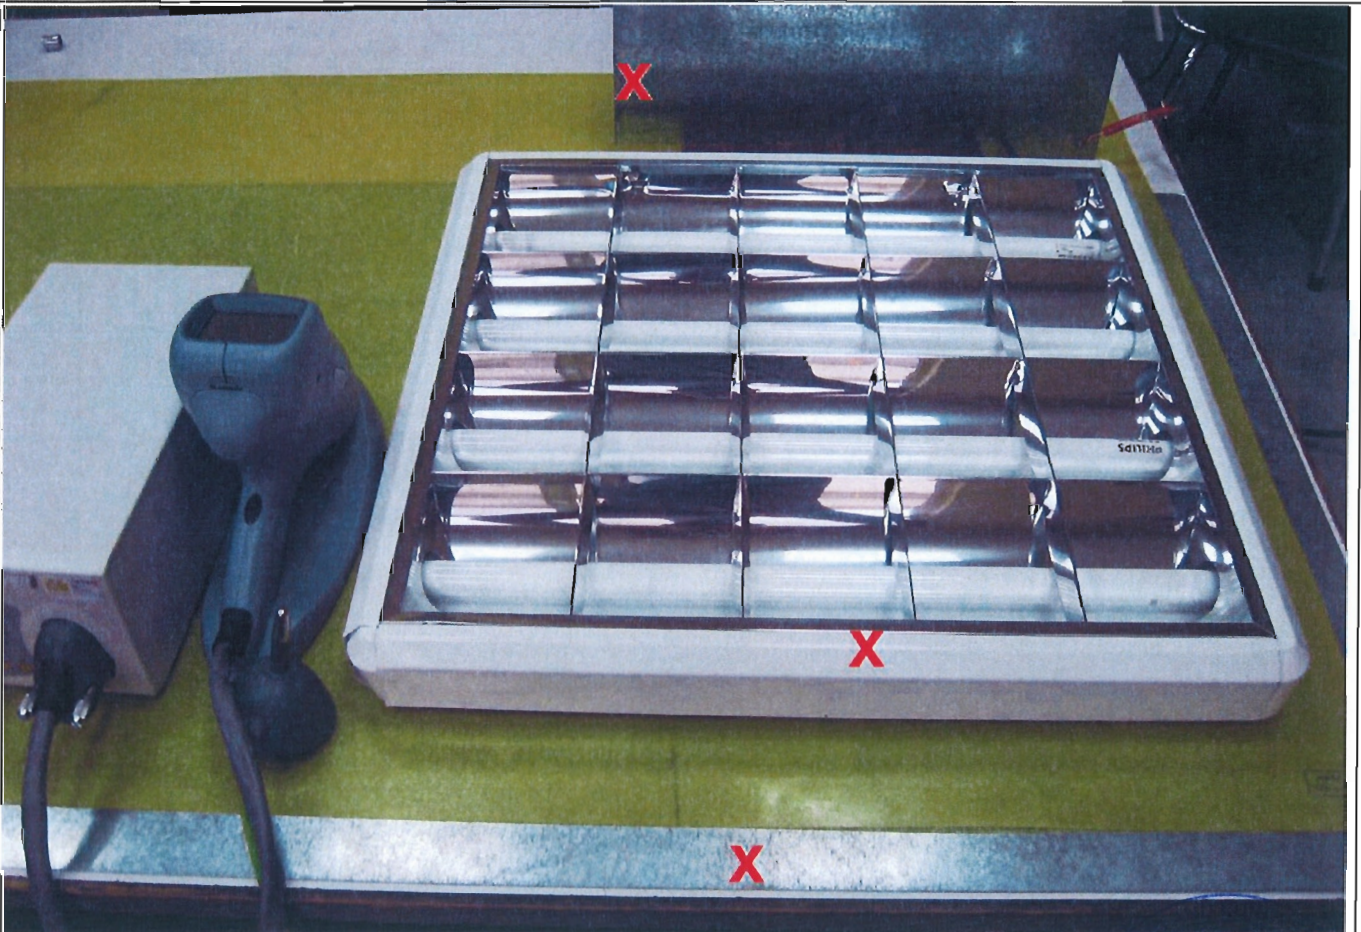

*The results showed in present test report concern tested sample only
 The test report could be reproduced as a whole only and after written permission of the laboratory*



2. ELECTRICAL FAST TRANSIENT/BURST IMMUNITY TEST

BDS EN 61547, τ. 5.5 – Applicability ,Table 6

BDS EN 61000-4-4, τ. 7 – Test setup

BDS EN 61000-4-4, τ. 8 – Test procedure

| | |
|---|--------------------------------------|
| Rise time | 5 ns ±30 % |
| Duration | 50 ns ± 30 % |
| Repetition frequency | 5 kHz |
| Burst duration | 15 ms ± 20 % за 5 kHz |
| Burst period | 300 ms ± 20 % |
| Time of application | 1 min for each polarity and coupling |
| Performance Criteria according to cl.6.3.4 and Table 15 of BDS EN 61547 | Criteria B |

| Pulse Application | Application | Level | Test Voltage V | Polarity | Result |
|---|------------------|-------|----------------|----------|-------------------|
| Between L and Ground plane | Coupling network | 1 | 500 | + | Pass (criteria A) |
| | | | | - | Pass (criteria A) |
| | | 2 | 1000 | + | Pass (criteria A) |
| | | | | - | Pass (criteria A) |
| Between neutral and Ground plane | Coupling network | 1 | 500 | + | Pass (criteria A) |
| | | | | - | Pass (criteria A) |
| | | 2 | 1000 | + | Pass (criteria A) |
| | | | | - | Pass (criteria A) |
| Between PE and Ground plane | Coupling network | 1 | 500 | + | Pass (criteria A) |
| | | | | - | Pass (criteria A) |
| | | 2 | 1000 | + | Pass (criteria A) |
| | | | | - | Pass (criteria A) |
| Between L, neutral, PE and Ground plane | Coupling network | 1 | 500 | + | Pass (criteria A) |
| | | | | - | Pass (criteria A) |
| | | 2 | 1000 | + | Pass (criteria A) |
| | | | | - | Pass (criteria A) |

Signal lines

| Pulse Application | Application | Level | Test Voltage V | Polarity | Result |
|-------------------|----------------|-------|----------------|----------|--------|
| - | Coupling clamp | 1 | 500 | + | - |
| | | | | - | - |
| - | Coupling clamp | 2 | 1000 | + | - |
| | | | | - | - |

Control lines

| Pulse Application | Application | Level | Test Voltage V | Polarity | Result |
|-------------------|----------------|-------|----------------|----------|--------|
| - | Coupling clamp | 1 | 500 | + | - |
| | | | | - | - |
| - | Coupling clamp | 2 | 1000 | + | - |
| | | | | - | - |

*The results showed in present test report concern tested sample only
The test report could be reproduced as a whole only and after written permission of the laboratory*





3. SURGE IMMUNITY TEST

BDS EN 61547, τ. 5.7 – Applicability ,Table 10
BDS EN 61000-4-5, τ. 7 – Test setup
BDS EN 61000-4-2, τ. 8 – Test procedure

| | | |
|---|--|----------------------------|
| Front time | 1,2 μs ± 30 % | |
| Time to half value | 50 μs ± 20 % | |
| Source impedance | Power line symmetrical Power line unsymmetrical | 2 Ω + 18 μF 12 Ω + 9 μF |
| Phase angles | 90°/ 270° | |
| Number of surges / polarity /phase angle | 5 | |
| Performance Criteria according to cl.6.3.4 and Table 15 of BDS EN 61547 | Criteria C | |

Power line symmetrical

| Pulse Application | Level | Test Voltage V | Polarity | Result |
|---------------------|-------|----------------|----------|-------------------|
| phase L – neutral N | 1 | 500 | + | Pass (criteria A) |
| | | | - | Pass (criteria A) |
| | 2 | 1000 | + | Pass (criteria B) |
| | | | - | Pass (criteria B) |

Power line unsymmetrical

| Pulse Application | Level | Test Voltage V | Polarity | Result |
|------------------------------|-------|----------------|----------|-------------------|
| phase L – protective earth | 1 | 500 | + | Pass (criteria A) |
| | | | - | Pass (criteria A) |
| | 2 | 1000 | + | Pass (criteria B) |
| | | | - | Pass (criteria B) |
| | 3 | 2000 | + | Pass (criteria B) |
| | | | - | Pass (criteria B) |
| neutral N - protective earth | 1 | 500 | + | Pass (criteria A) |
| | | | - | Pass (criteria A) |
| | 2 | 1000 | + | Pass (criteria B) |
| | | | - | Pass (criteria B) |
| | 3 | 2000 | + | Pass (criteria B) |
| | | | - | Pass (criteria B) |

*The results showed in present test report concern tested sample only
The test report could be reproduced as a whole only and after written permission of the laboratory*





4. RATED POWER FREQUENCY MAGNETIC FIELD

BDS EN 61547, τ. 5.4 – Applicability ,Table 3

BDS EN 61000-4-8 τ. 7 – Test setup

BDS EN 61000-4-8 τ. 8 – Test procedure

Performance Criteria according to cl.6.3.3
and Table 15 of BDS EN 61547

Criteria A

| Standard inductive coil | Orientation of standard inductive coil | Level | Field strength in the centre for all other inductive coils | Current in the coil (a coil with 10 windings) | Result |
|-------------------------|--|-------|--|---|-------------------|
| 1 m x 1 m | X | 2 | 3 A/m | 3,45 A | Pass (criteria A) |
| 1 m x 1 m | Y | 2 | 3 A/m | 3,45 A | Pass (criteria A) |
| 1 m x 1 m | Z | 2 | 3 A/m | 3,45 A | Pass (criteria A) |

*The results showed in present test report concern tested sample only
The test report could be reproduced as a whole only and after written permission of the laboratory*





5. Voltage dips, short interruptions and voltage variations immunity tests

5.1 Voltage dips immunity tests

BDS EN 61547, τ. 5.8 – Applicability ,Table 11

BDS EN 61000-4-11 τ. 7 – Test setup

BDS EN 61000-4-11 τ. 8 – Test procedure

BDS EN 61000-4-11 τ. 8.2.1 – Testing for each selected combination of test level and duration with a sequence of three dips with intervals of 10 s minimum (between each test event)

Performance Criteria according to cl.6.3.4 and Table 15 of BDS EN 61547

Criteria C

| Voltage test levels (% of rated voltage) | Duration (cycles) | Phase angle synchronization | Result |
|--|----------------------|-----------------------------|-------------------|
| 70 % | 10 cycles | 0° | Pass (criteria B) |

5.2 Short interruptions immunity tests

BDS EN 61547, τ. 5.8 – Applicability ,Table 12

BDS EN 61000-4-11 τ. 7 – Test setup

BDS EN 61000-4-11 τ. 8 – Test procedure

BDS EN 61000-4-11 τ. 8.2.1 – Testing for each selected combination of test level and duration with a sequence of three interruptions with intervals of 10 s minimum (between each test event)

Performance Criteria according to cl.6.3.4 and Table 15 of BDS EN 61547

Criteria B

| Voltage test levels (% of rated voltage) | Duration (cycles) | Phase angle synchronization | Result |
|--|----------------------|-----------------------------|-------------------|
| 0 % | 0,5 cycles | 0° | Pass (criteria B) |

*The results showed in present test report concern tested sample only
The test report could be reproduced as a whole only and after written permission of the laboratory*





USED TECHNICAL EQUIPMENTS:

| | Appliance | Type | Manufacturer | Identity № | Last calibration date |
|-----|------------------------------------|---|---|---|------------------------------|
| 1. | ESD - Generator | NSG438 | TESEQ Switzerland | 988 | 14.03.2012 |
| 2. | EFT/B - Generator | NSG 2050 INA 2050 PNW 2225 CDN 133 | Schaffner Electrotest GmbH, Germany | 200902-653LU 200906-578LU 200838-570LU 34460 | 14.03.2012 |
| 3. | Surge - Generator | NSG 2050 INA 2050 PNW 2050 CDN 133 | Schaffner Electrotest GmbH, Germany | 200902-653LU 200906-578LU 200911-636LU 34460 | 16.03.2012 |
| 4. | Digital multimeter | UNIGOR 390 | LEM Austria | PI 3288 | 08.07.2011 |
| 5. | Voltage Generator | GL 01-16-230 | Neosvet Bulgaria | 0001 | - |
| 6. | Power Quality Analyzer | 435 | Fluke Netherlands | DM 9881064 | 08.11.2011 |
| 7. | Thermometer-higrometer | 177-H1 | TESTO Germany | 01320300/902 | 19.04.2012 |
| 8. | EMI – receiver 9 kHz ÷ 1000 MHz | SCR 3501 | Schaffner Electrotest GmbH, Germany | 522 | 07.07.2011 |
| 9. | Large loop antenna 2m | RF300 | Laplace Instruments LTD U.K. | 9123 | 12.03.2013 |
| 10. | Coupling/Decoupling network | CDN M2+M3 | Frankonia EMC Test - Systems | A2210229 | 18.04.2013 |

TEST PERFORMER: 1.

/ T. Hristov /



2.

/D. Chavalinov /

CHIEF LABORATORY :

/ T. Hristov /